

NEW SPIRIT NATURALS, INC.
615 West Allen Avenue, San Dimas, CA 91773, USA

MANUFACTURING CERTIFICATE

We hereby certify the following by the best of our knowledge and belief. "Colloidal Silver" is a trademark of New Spirit Naturals, Inc. and is manufactured in the United States of New Spirit Naturals, Inc. All products are retailed in the United States by New Spirit Naturals, Inc. and supplied by New Spirit Naturals, Inc. for distribution in the International Market. New Spirit Naturals, Inc. has been producing and supplying nutritional supplements and vitamins for many years without any problems. All products are manufactured in a GMP (Good Manufacturing Practice) FDA Registered Establishment (#2032763). New Spirit Naturals is also licensed by the California Department of Health Services, Food and Drug Branch (Drug Manufacturing License #18941). We have strict quality control, and we are monitored and licensed by the State of California, Department of Health Services, Food and Drug Branch.

I	U.S. Supplier:	New Spirit Naturals, Inc. 615 W. Allen Ave. San Dimas, CA 91773, USA
II	Manufacturer:	New Spirit Naturals, Inc. 615 W. Allen Ave. San Dimas, CA 91773, USA
III	Distributor:	Viterity Global, LLC
IV	Product Name:	Colloidal Silver
	A) Composition:	See Attached
	B) State:	Liquid
	C) Classification:	Nutritional Supplement
	D) Effect:	Dietary Supplement
	E) Directions:	Use per label directions
	F) Precautions:	None
	G) Package Size & Type:	4 fl. oz. (118 ml) plastic bottle
	H) Storage:	Cool dry place, 15°C-25°C
	I) Expiration:	Appears on each label and is based on a 3 year period from date of manufacture

CONTAINS NO DRUG (NARCOTIC) & GENETICALLY MODIFIED INGREDIENTS BASED ON CERTIFICATE OF ANALYSIS



Dr. Larry J. Milam H.M.D., Ph.D. (President)

Date: September 26, 2023

NEW SPIRIT NATURALS, INC.
615 West Allen Avenue, San Dimas, CA 91773, USA

CERTIFICATE OF ANALYSIS

The Certificate of Analysis and all the contents herein remains the property of New Spirit Naturals, Inc. and is not to be disclosed to any third party, except Government Agencies, without the expressed written permission of New Spirit Naturals, Inc. of San Dimas, California, U.S.A. This certificate is considered intellectual property of New Spirit Naturals, Inc. Any violation of use of this certificate as stated above may subject the violator to civil and criminal penalties and actions to the full extent of the laws of the United States of America and the State of California. By accepting this Certificate the accepting party/parties agree to the above conditions.

MANUFACTURER: New Spirit Naturals, Inc.
PRODUCT NAME: Colloidal Silver
PRODUCT #: 266
PHYSICAL FORM: Transparent Liquid
COLOR: Clear
ASSAY METHOD: By input
MANUFACTURING METHOD:
1. Place Silver bar in tank
2. Add deionized water
3. Add electrical charge until 5/15 parts per million is achieved
4. Check for ppm in Lab (Quality Control)
5. Bottle, Label and Code finished product
6. Place Silver bar in tank

<u>INGREDIENTS PER SERVING</u>	<u>WEIGHT</u>	<u>% CONTENT</u>
ACTIVE:		
Colloidal Silver (5/15 parts per million)	0.000000006 g	0.0000001 %
SUBTOTAL:	0.000006 MG	
NON-ACTIVE:		
Deionized water	5.999999994 g	99.9999999 %
TOTAL:	6.00 G	100.00 %

No preservatives, color, flavoring or fragrance added

INSTRUCTIONS FOR USE: One teaspoon daily. Children: 1/4 - 1/2 adult dose. Maybe mixed with water or juice, preferably between meals. May also be applied topically.
CONTRA-INDICATIONS: None
STORAGE: Keep in a cool dry condition away from light and heat, 15°C-25°C
SHELF LIFE: 3 years

This is to certify that the above particulars in this certificate are true and correct.




Dr. Larry J. Milam *D.C., Ph.D. (President)*

Date: *September 26, 2023*

NEW SPIRIT NATURALS, INC.
615 West Allen Avenue, San Dimas, CA 91773, USA

QUALITY CONTROL CERTIFICATE

PRODUCT: Colloidal Silver
PRODUCT#: 266
LOT#: 231932L

ANALYSIS PER SERBING	CLAIM	FOUND*
Colloidal Silver (5/15 parts per million)	0.000000006 g	100.00 %
Deionized water	5.999999994 g	100.00 %

DESCRIPTION: Transparent Liquid
IDENTIFICATION: Positive

*Based on manufacturer certificate of analysis

ASSAY METHOD:

By input
31 July, 2026

EXPIRATION DATE:


TOTAL MICROBIOLOGICAL

STANDARDS:		RESULTS:	
Plate count:	<30	Plate count:	<10
Yeast & mold:	<10	Yeast & mold:	<10
Salmonella:	Negative	Salmonella:	Negative
Staphylococcus A:	Negative	Staphylococcus A:	Negative
Pseudomonas Aeruginosa:	Negative	Pseudomonas Aeruginosa:	Negative
E. coli:	Negative	E. coli:	Negative

BASED ON PHYSICAL EXAMINATION

LABORATORY MANAGER _____

Will D.

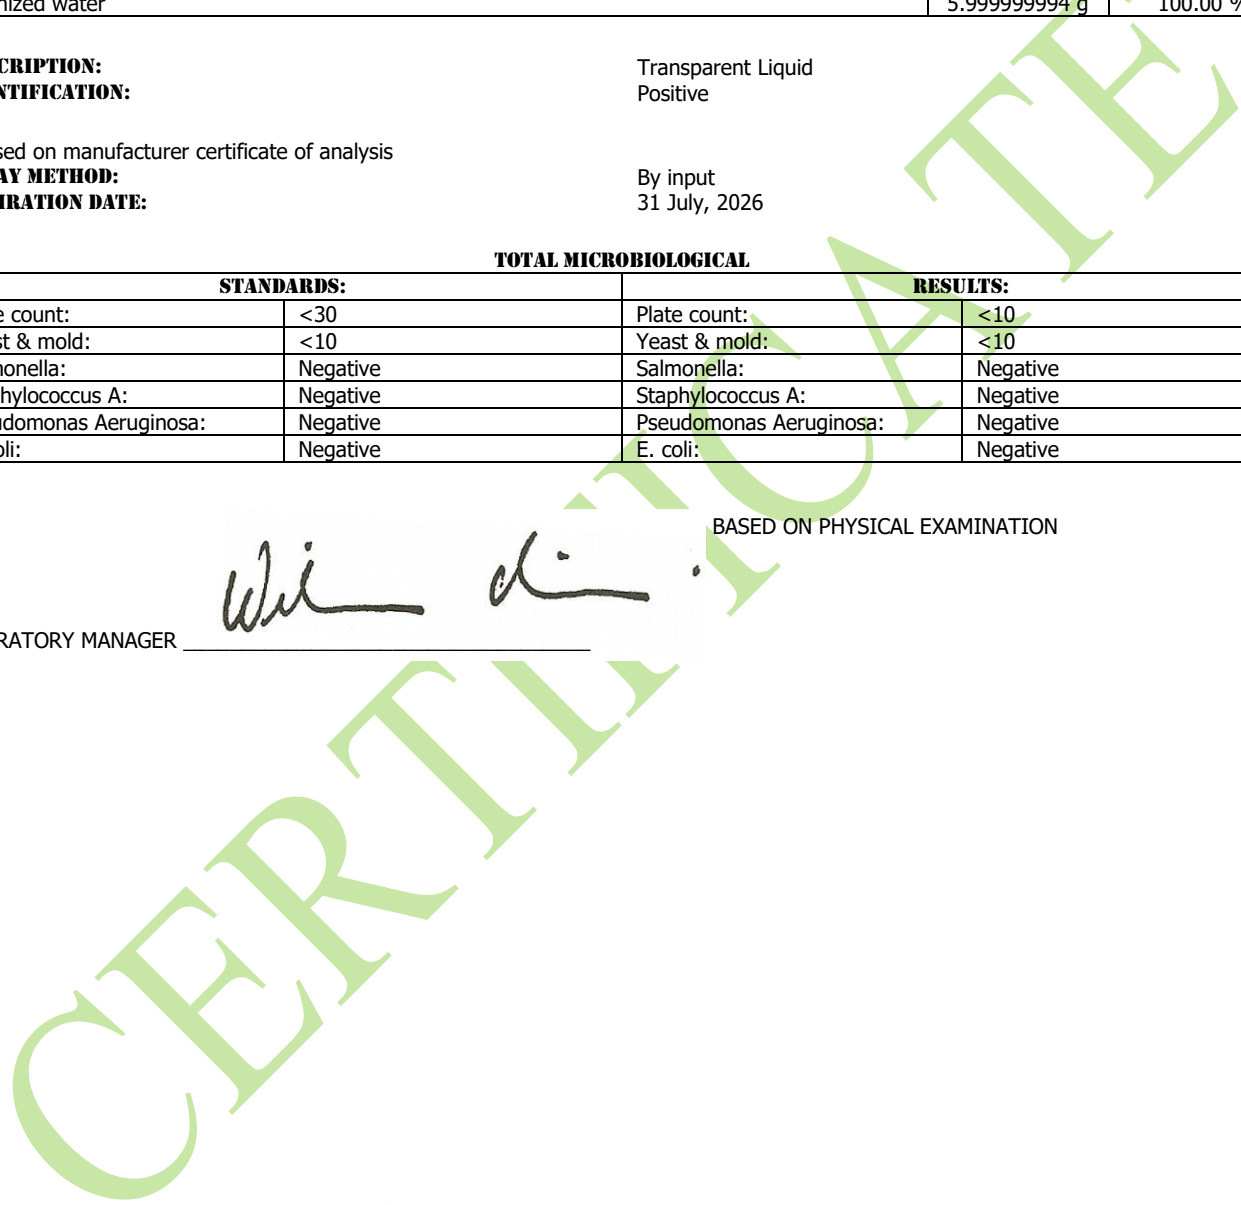

Larry J. Milam



Dr. Larry J. Milam Ph.D., Ph.D. (President)

Date: *September 26, 2023*